


Application Note #0001

Protein Standards - Reverse Phase

Column: FM-PhEs
Dimensions: 100 x 3.2mm ID
Order No.:
Detection: 200 nm
Flow Rate (mL/min): 1.500
Injection Volume: 10ul
Column Temperature: 35.0
Sample Loop Volume: 100uL

Elution Type: Gradient
Eluent A: 0.1% TFA in H2O
Eluent B: 0.06% TFA in ACN

Gradient Profile:	Step Number	Time (min)	%A	%B
	1	0	85	15
	2	6	40	60
	3	8	85	15

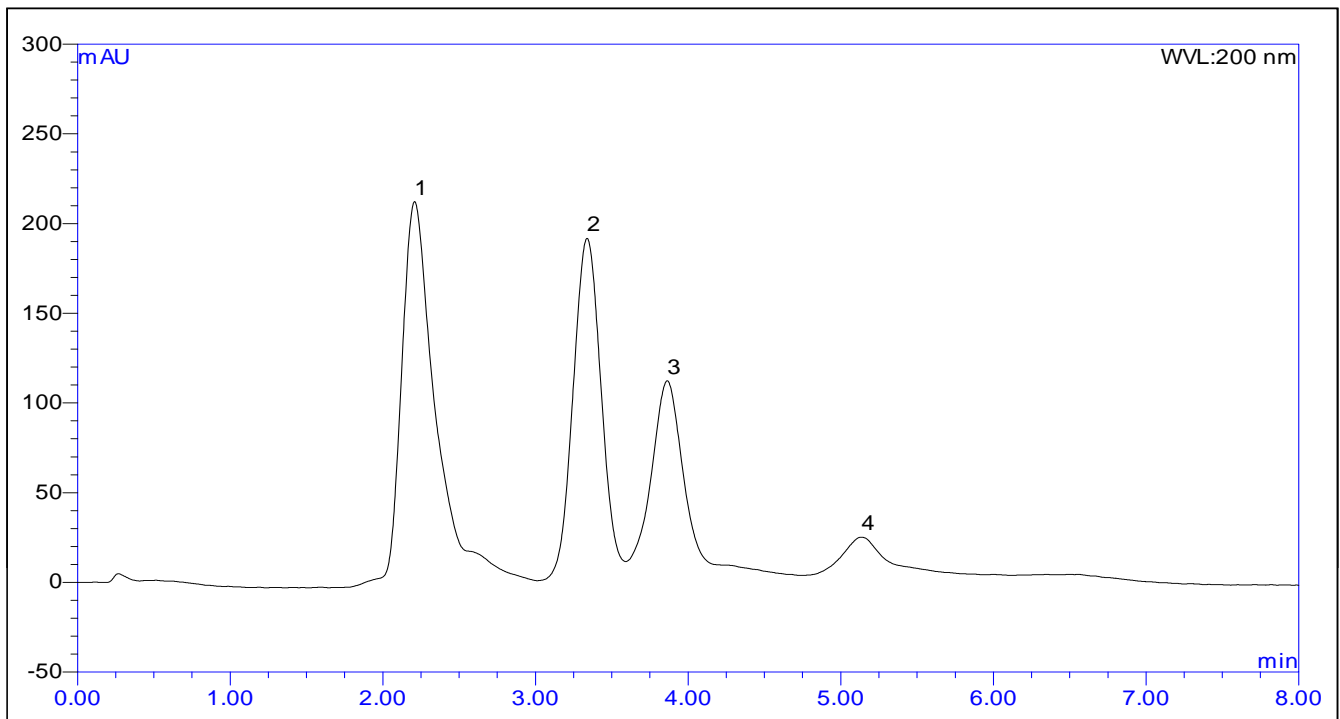

ANALYTES:

No.	Peak Name	Sample Conc.
1	Rnase A	0.19ug/ml
2	Lysozyme	0.19ug/ml
3	Myoglobin	0.19ug/ml
4	Ovalbumin	0.19ug/ml